
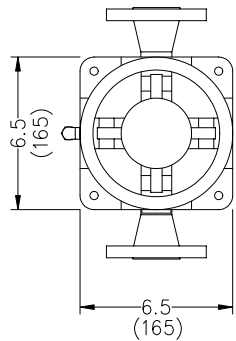
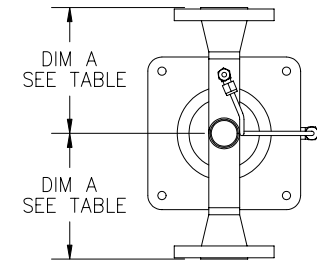
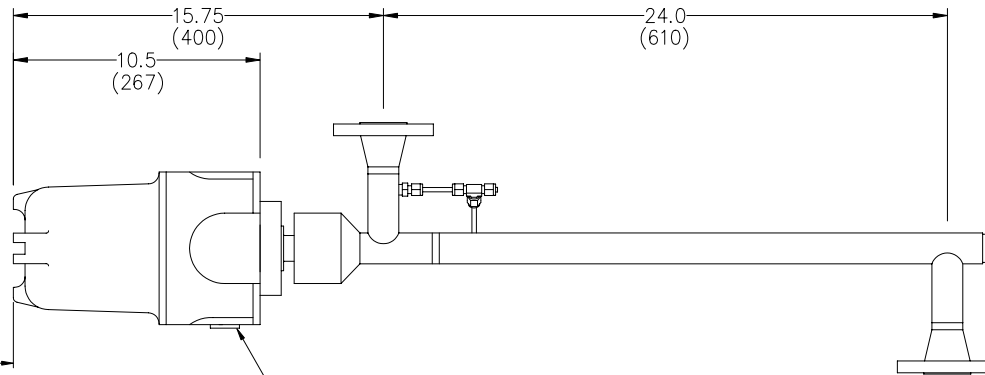


REV	DATE	ECO	COMMENTS
A	06/04/03	169	ADD METRIC UNITS

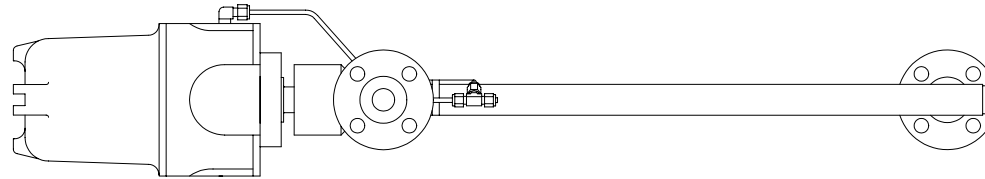


RECOMMENDED MINIMUM CLEARANCE FOR ACCESS

0.75-14 NPT REDUCING BUSHING (SUPPLIED)

NOTES:

- 1 ALL DIMENSIONS GIVEN IN INCHES MILLIMETER DIMENSIONS SHOWN IN ()
- 2 FLANGES ARE 1 INCH RAISED FACE SCHEDULE 80 BORE, 316L STAINLESS STEEL
- 3 PIPE IS 1 INCH, SCHEDULE 80, 316L STAINLESS STEEL
- 4 WEIGHT: SEE TABLE

FLANGE SIZE	DIMENSION "A"	WEIGHT (LBS) (KG)
ANSI 150	5.3 (135)	32 15
ANSI 300	5.6 (142)	35 16
ANSI 600	5.9 (150)	35 16
ANSI 900	6.3 (160)	44 20

 PHASE DYNAMICS, INC RICHARDSON, TEXAS	
TITLE INSTALLATION, 1 INCH Z CONFIG RAISED FACE FLANGES	
SIZE B	DWG. NO. 0070-00170-000
REV A	DATE 03/02/00
© PHASE DYNAMICS, INC.	